

METHOD AND APPARATUS FOR DEMODULATING SIGNALS IN A
PULSE OXIMETRY SYSTEM

Diab et al.

Appl. No.: Unknown

Atty Docket: MASIMO.CP1DV2

1/18

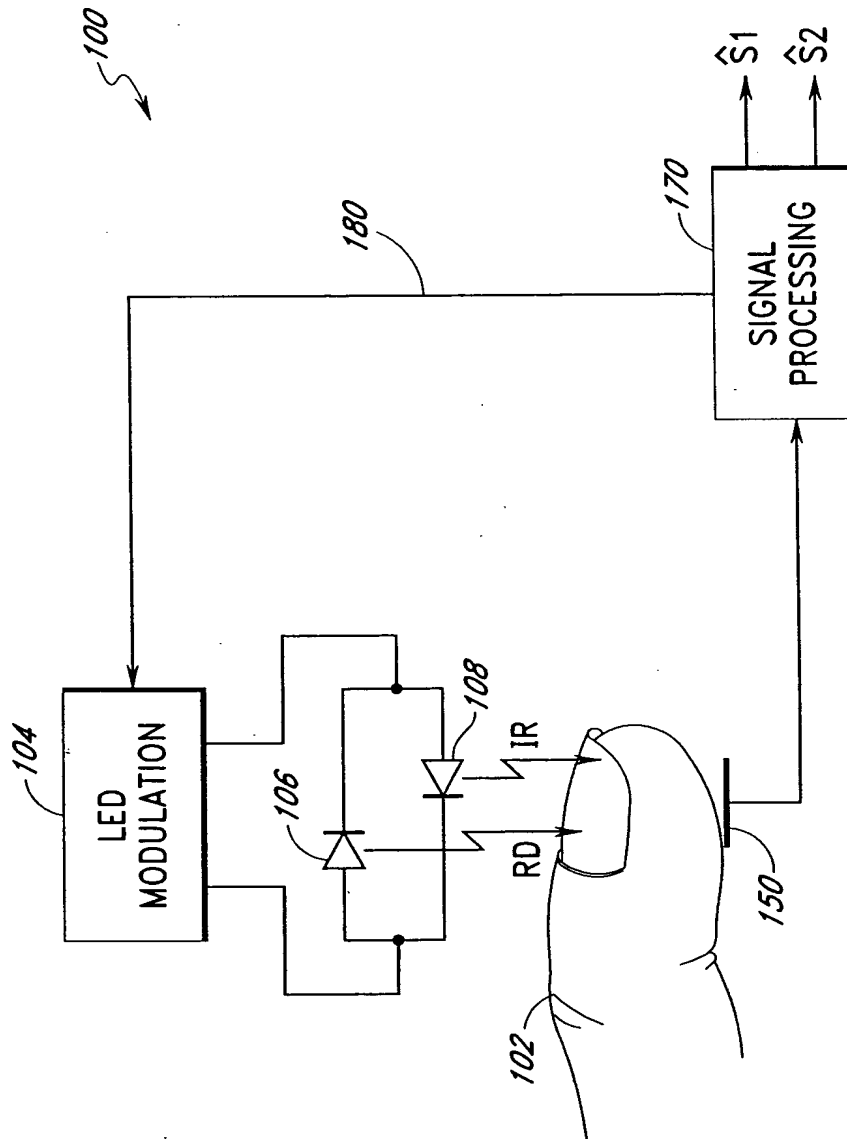


FIG. 1


METHOD AND APPARATUS FOR DEMODULATING SIGNALS IN A
PULSE OXIMETRY SYSTEM

Diab et al.

Appl. No.: Unknown

Atty Docket: MASIMO.CP1DV2

FIG. 2

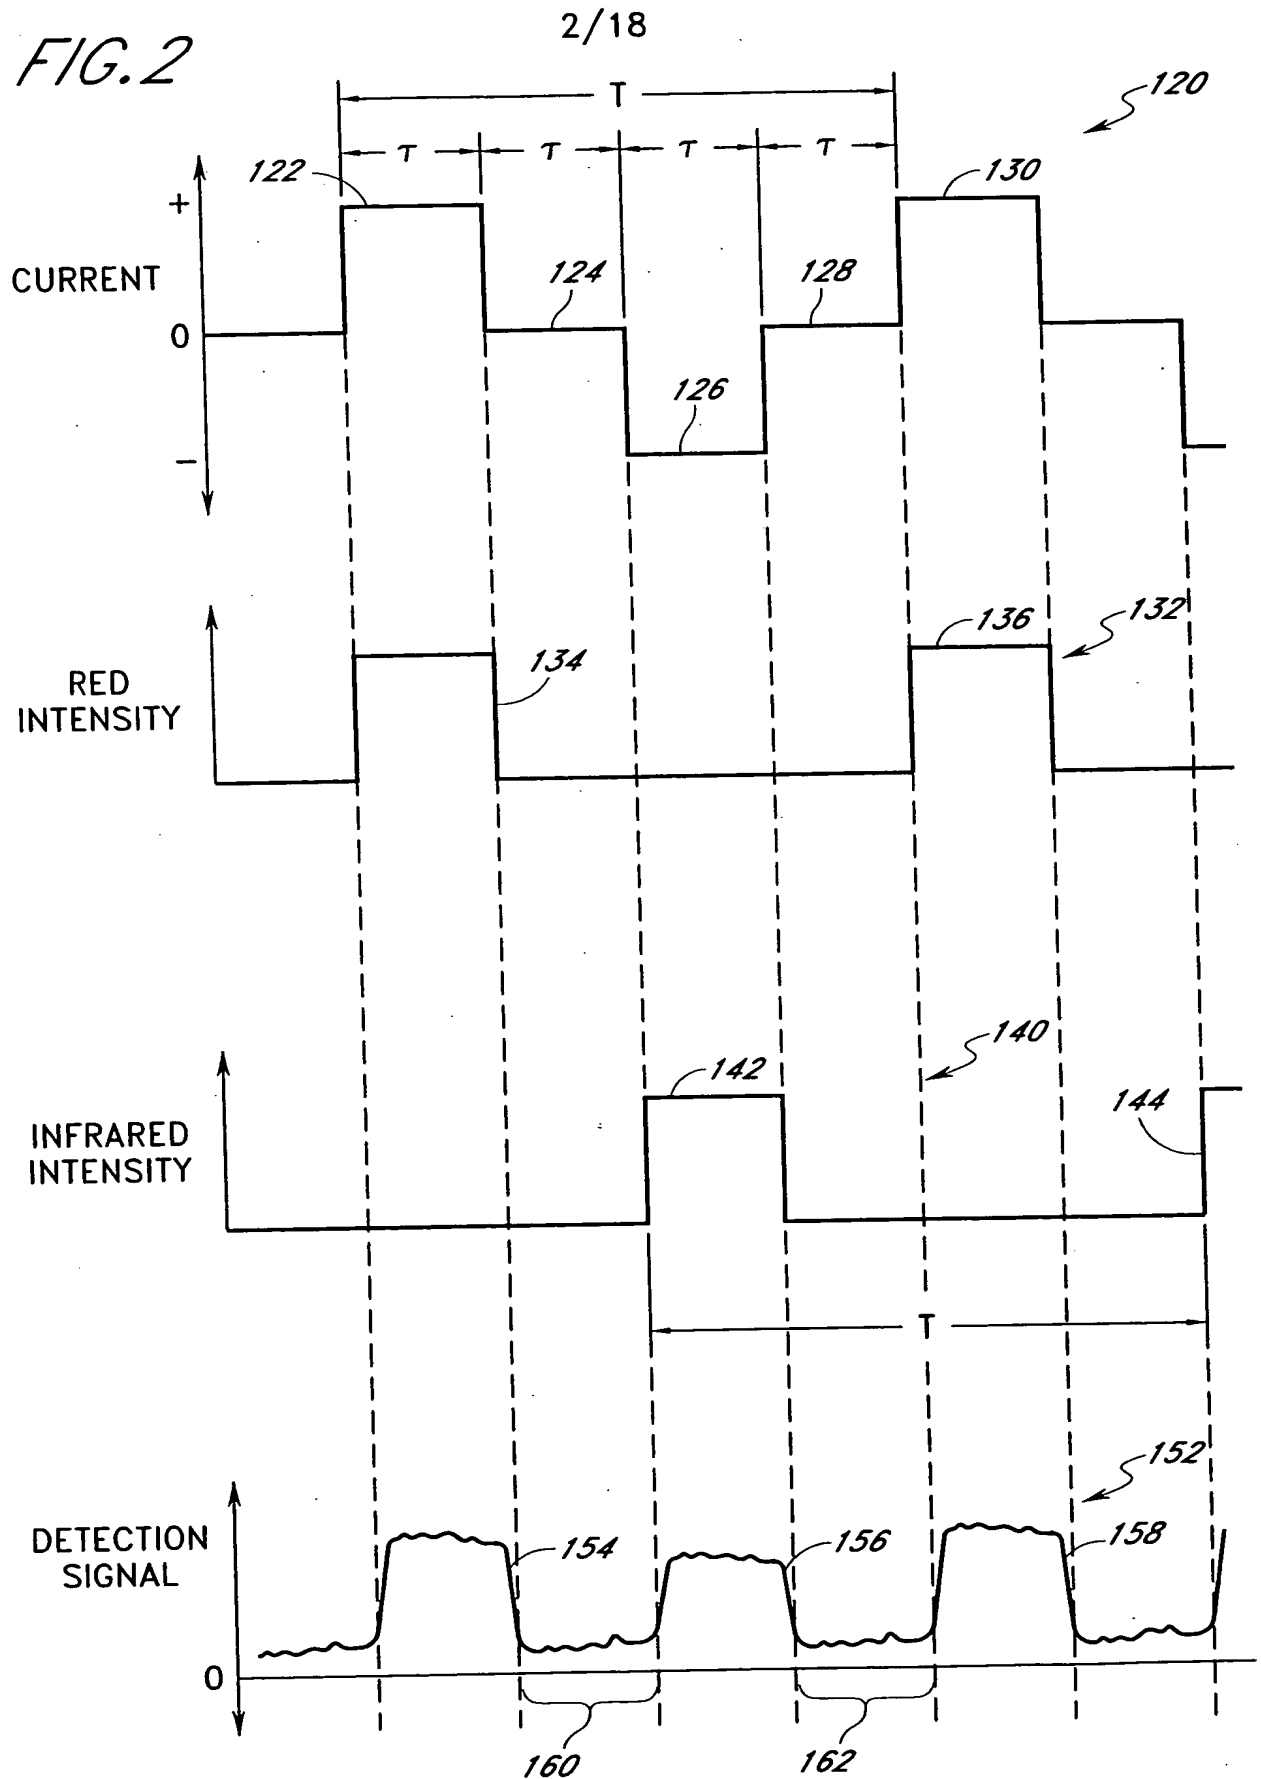

METHOD AND APPARATUS FOR DEMODULATING SIGNALS IN A
PULSE OXIMETRY SYSTEM

Diab et al.

Appl. No.: Unknown

Atty Docket: MASIMO.CP1DV2

3/18

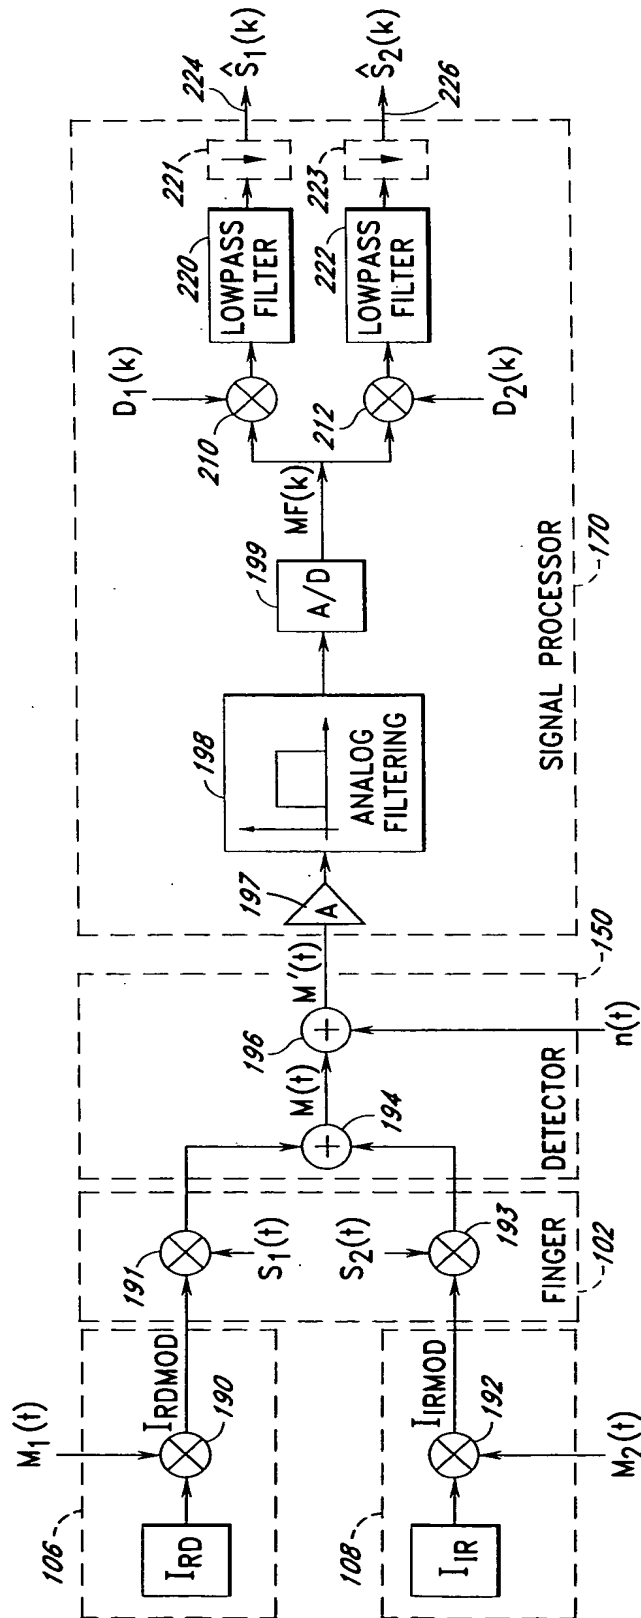


FIG. 3

METHOD AND APPARATUS FOR DEMODULATING SIGNALS IN A
PULSE OXIMETRY SYSTEM

Diab et al.

Appl. No.: Unknown

Atty Docket: MASIMO.CP1DV2

4/18

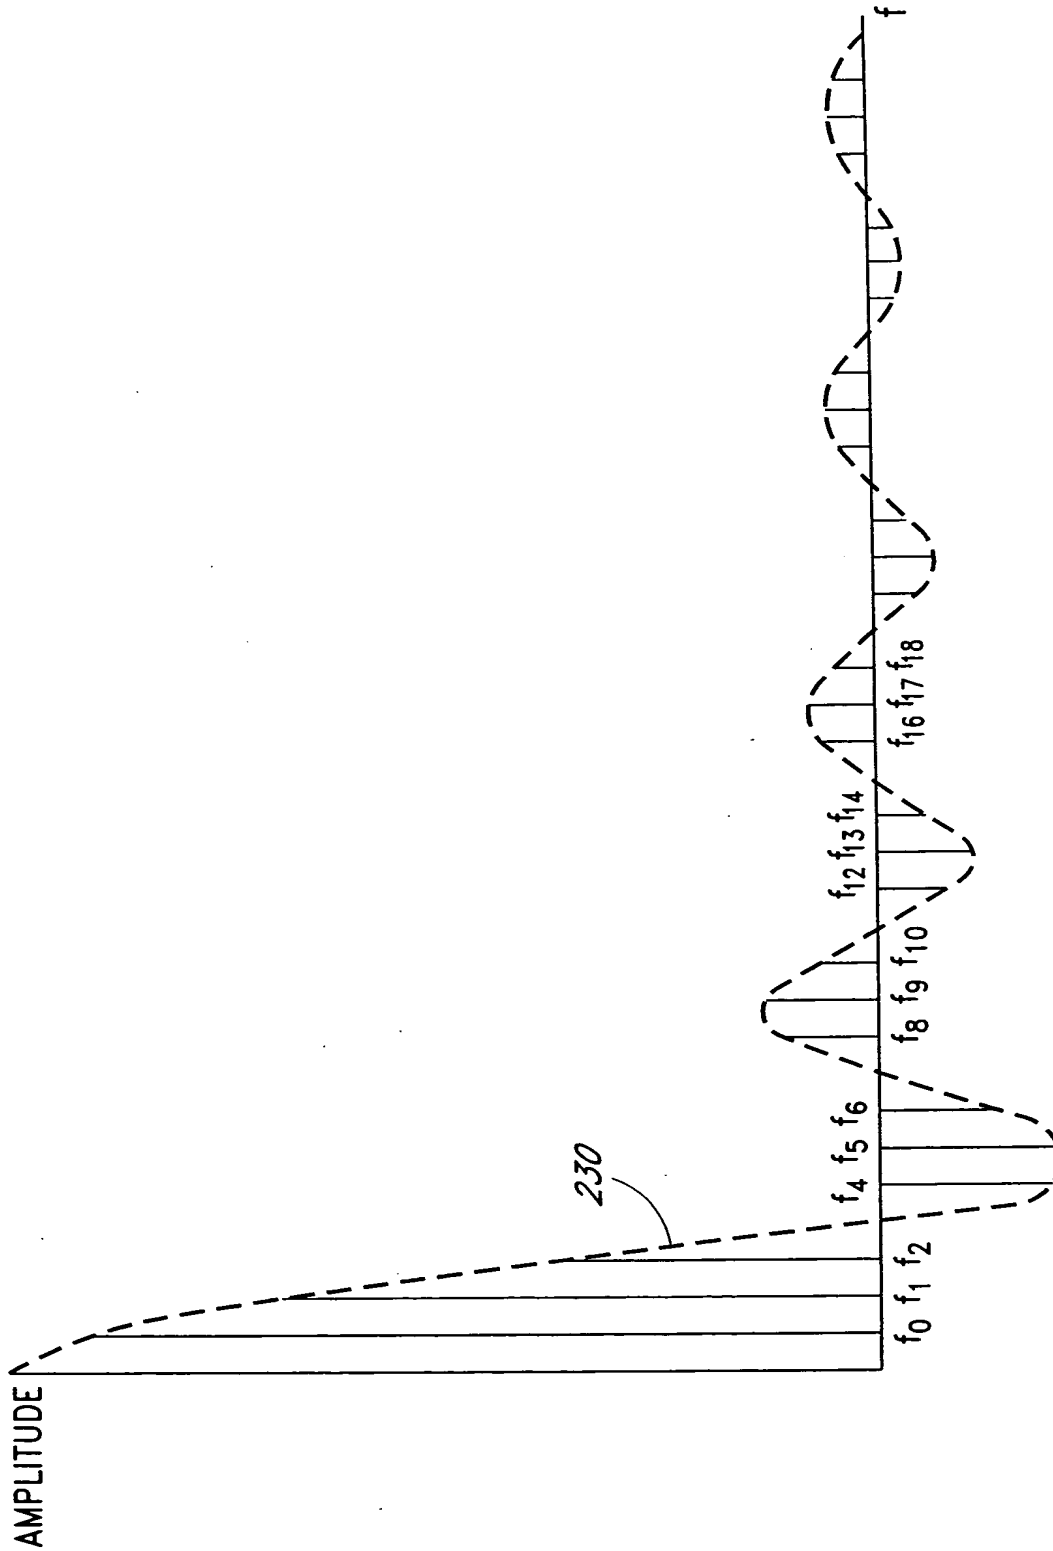


FIG. 4

5/18

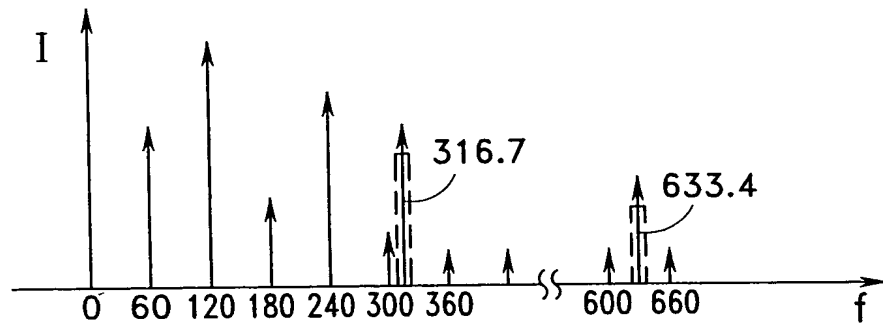


FIG. 5

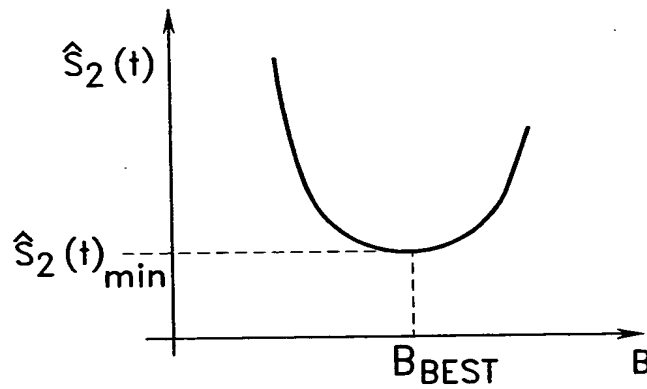


FIG. 6

METHOD AND APPARATUS FOR DEMODULATING SIGNALS IN A
PULSE OXIMETRY SYSTEM

Diab et al.

Appl. No.: Unknown

Atty Docket: MASIMO.CP1DV2

6/18

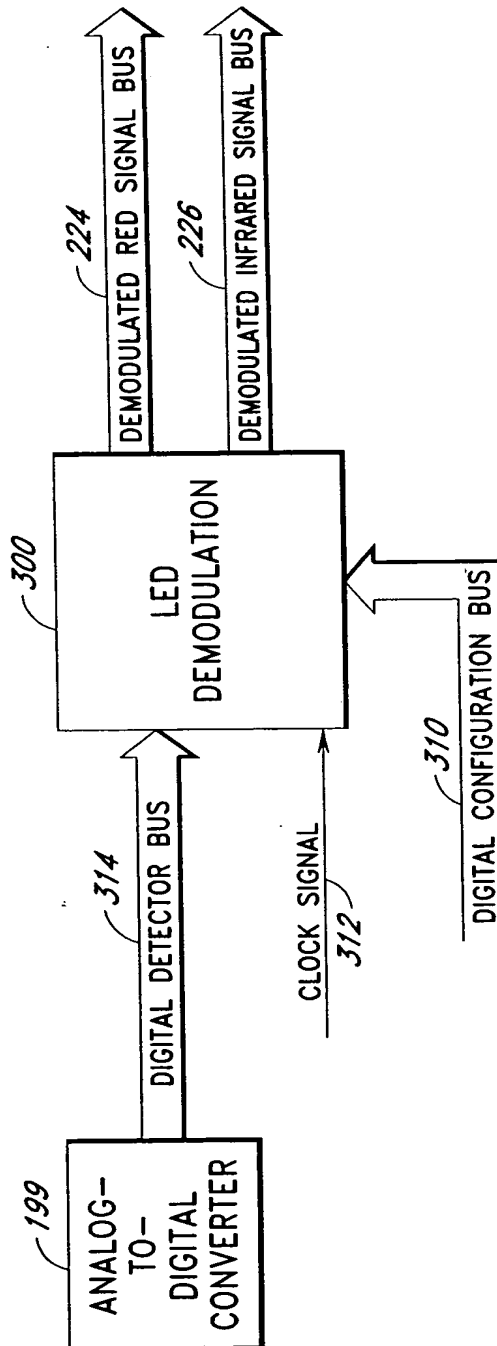


FIG. 7

METHOD AND APPARATUS FOR DEMODULATING SIGNALS IN A
PULSE OXIMETRY SYSTEM

Diab et al.

Appl. No.: Unknown

Atty Docket: MASIMO.CP1DV2

7/18

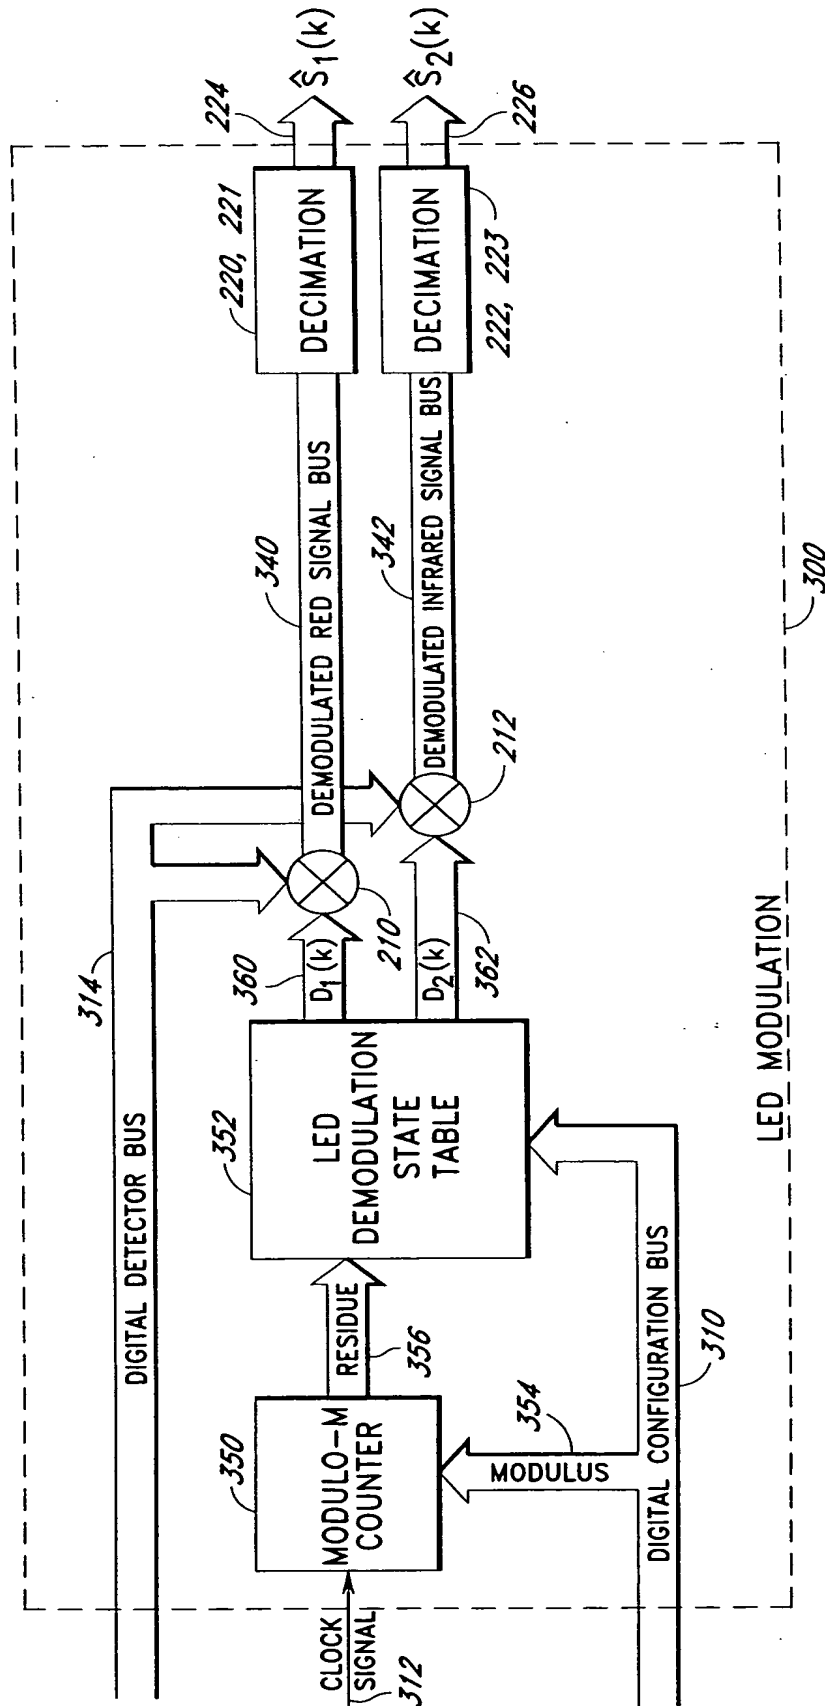


FIG. 8

METHOD AND APPARATUS FOR DEMODULATING SIGNALS IN A
PULSE OXIMETRY SYSTEM

Diab et al.

Appl. No.: Unknown

Atty Docket: MASIMO.CP1DV2

8/18



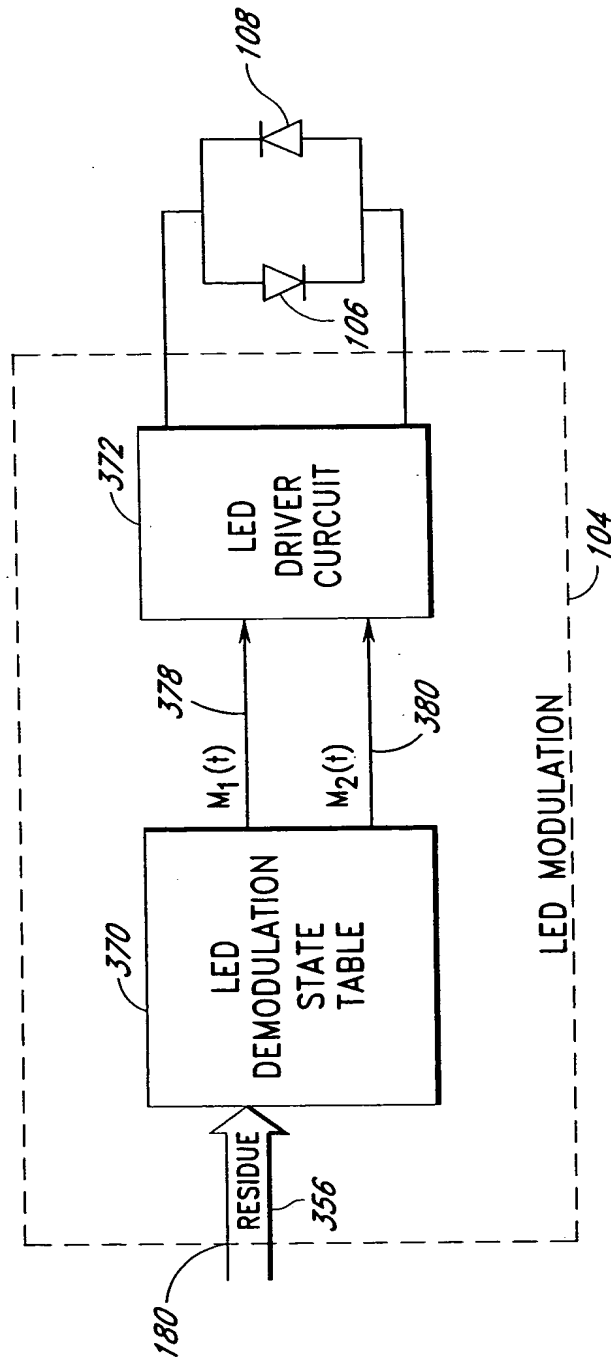


FIG. 9

9/18

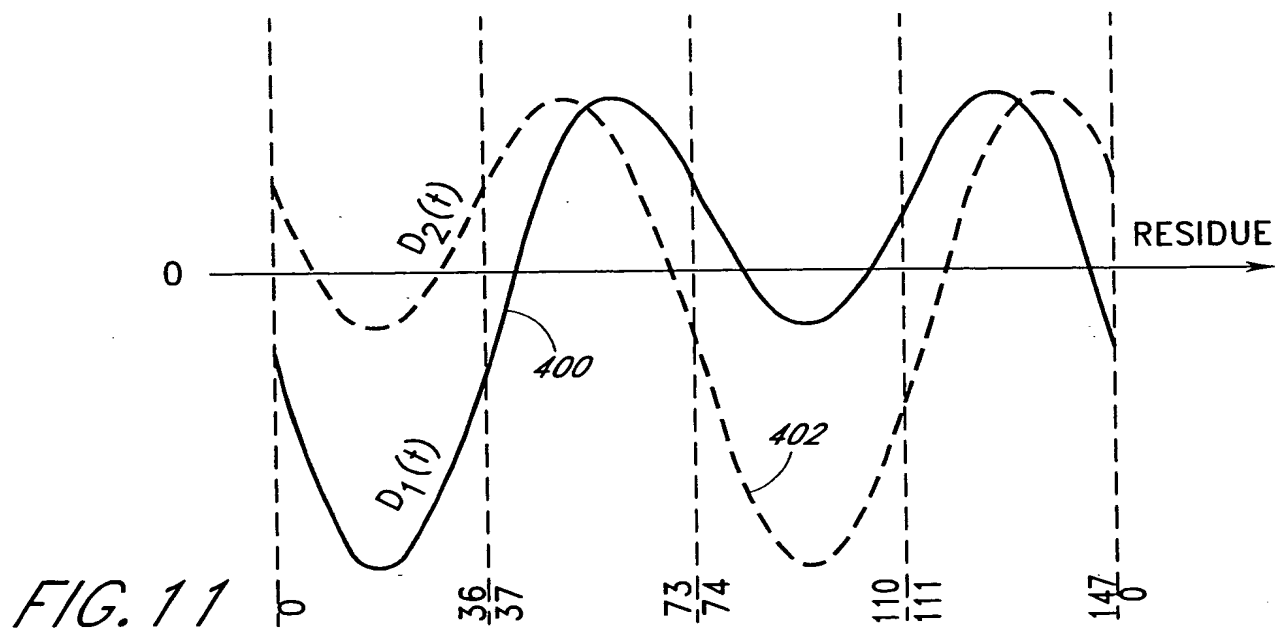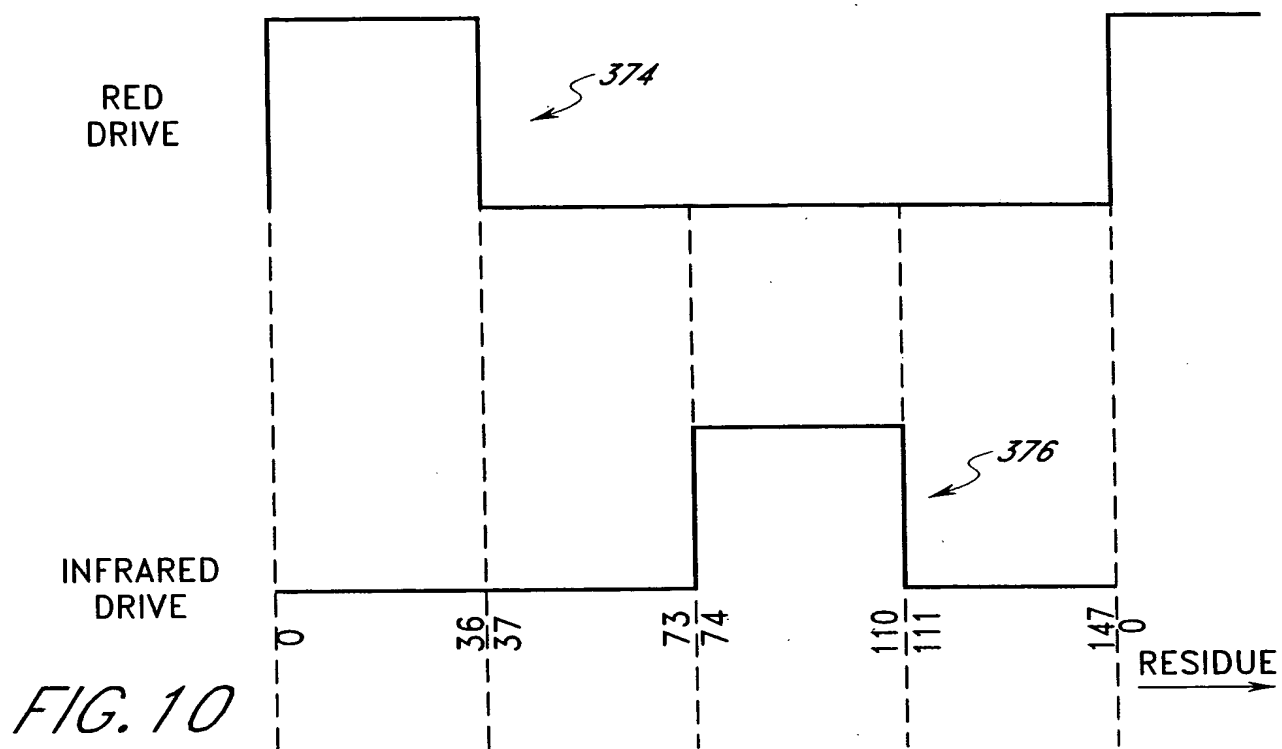

METHOD AND APPARATUS FOR DEMODULATING SIGNALS IN A
PULSE OXIMETRY SYSTEM

Diab et al.

Appl. No.: Unknown

Atty Docket: MASIMO.CP1DV2

10/18

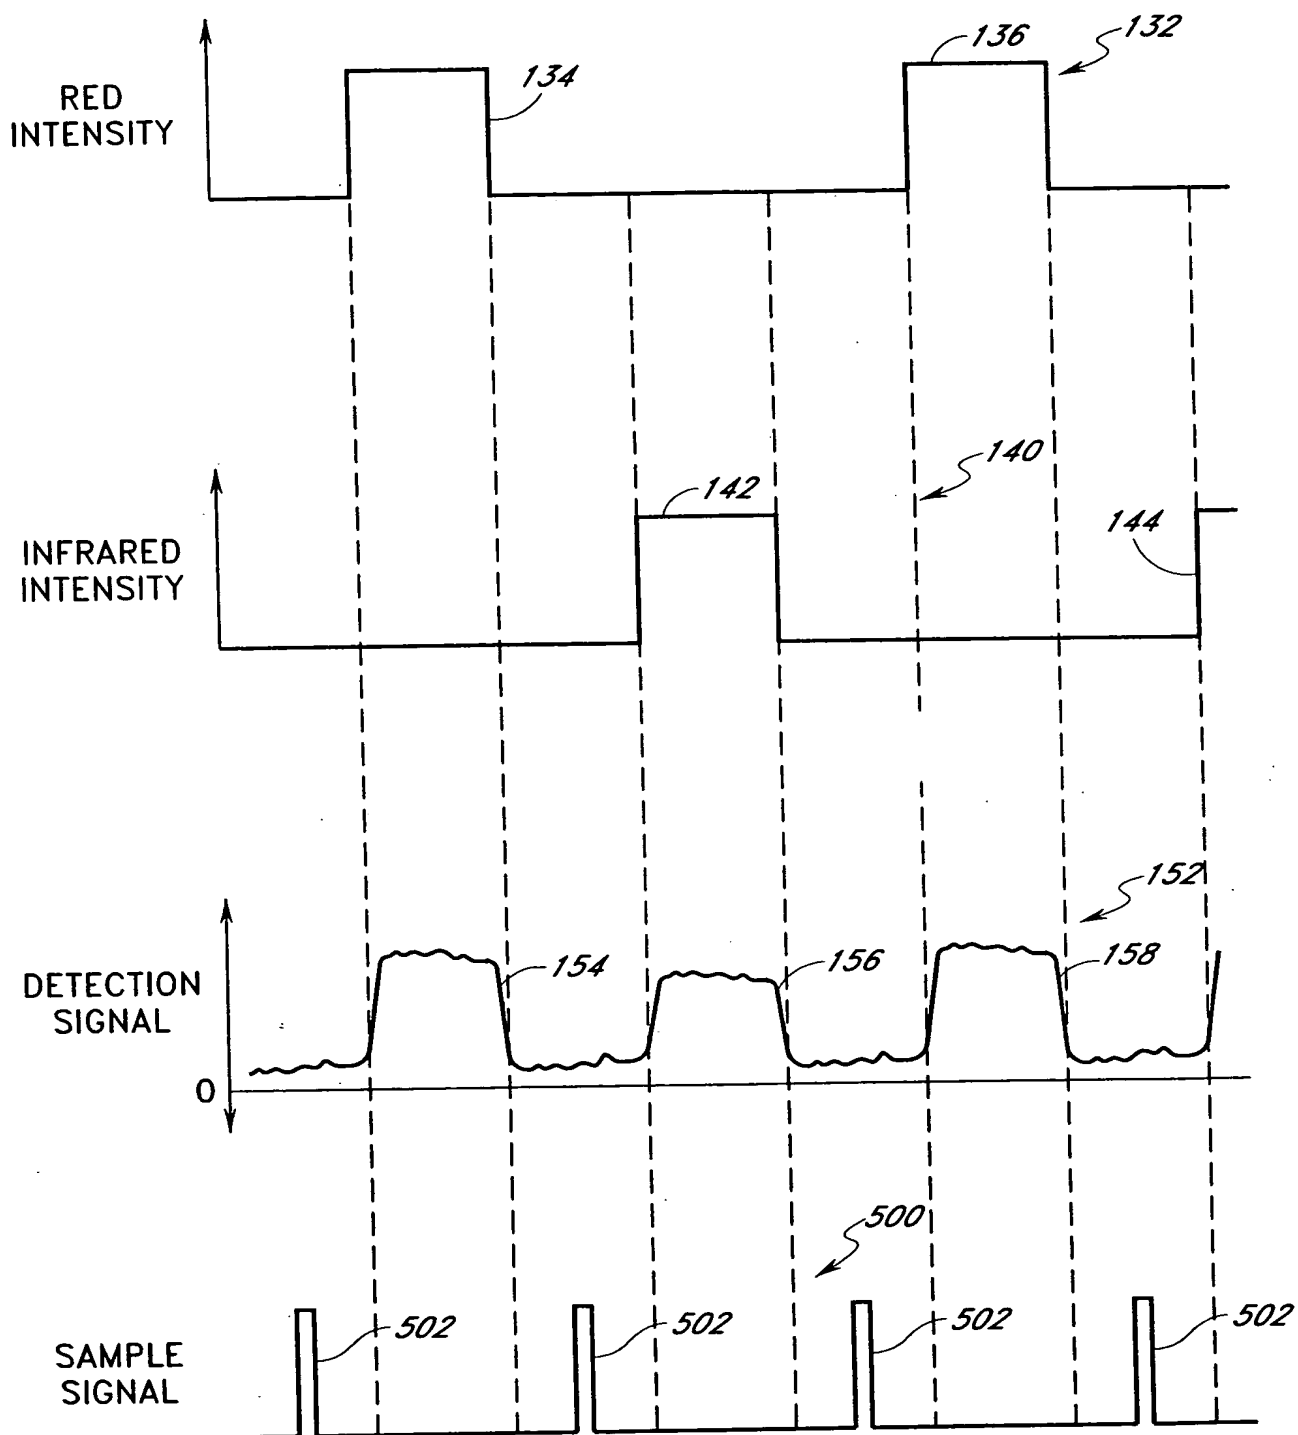


FIG. 12

METHOD AND APPARATUS FOR DEMODULATING SIGNALS IN A
PULSE OXIMETRY SYSTEM

Diab et al.

Appl. No.: Unknown

Atty Docket: MASIMO.CP1DV2

11/18

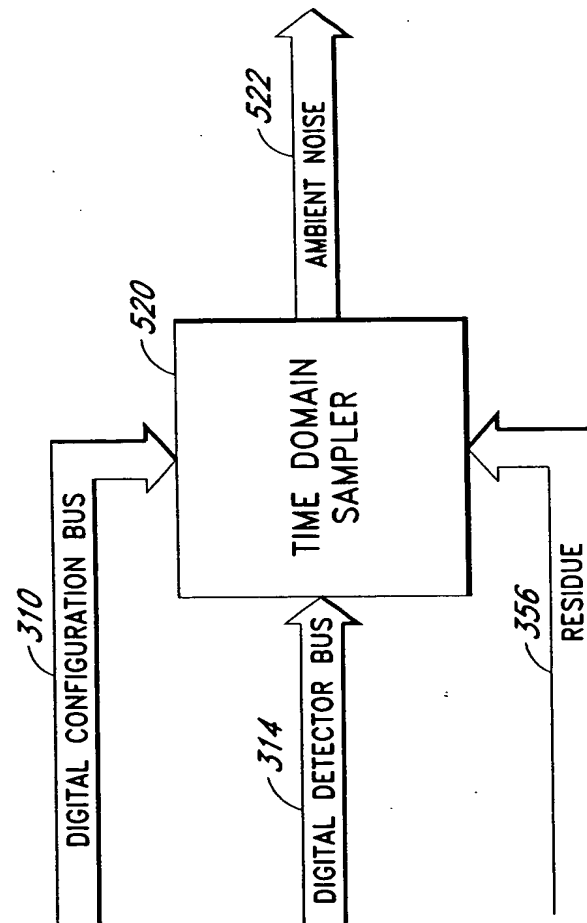


FIG. 13

METHOD AND APPARATUS FOR DEMODULATING SIGNALS IN A
PULSE OXIMETRY SYSTEM

Diab et al.

Appl. No.: Unknown

Atty Docket: MASIMO.CP1DV2

12/18

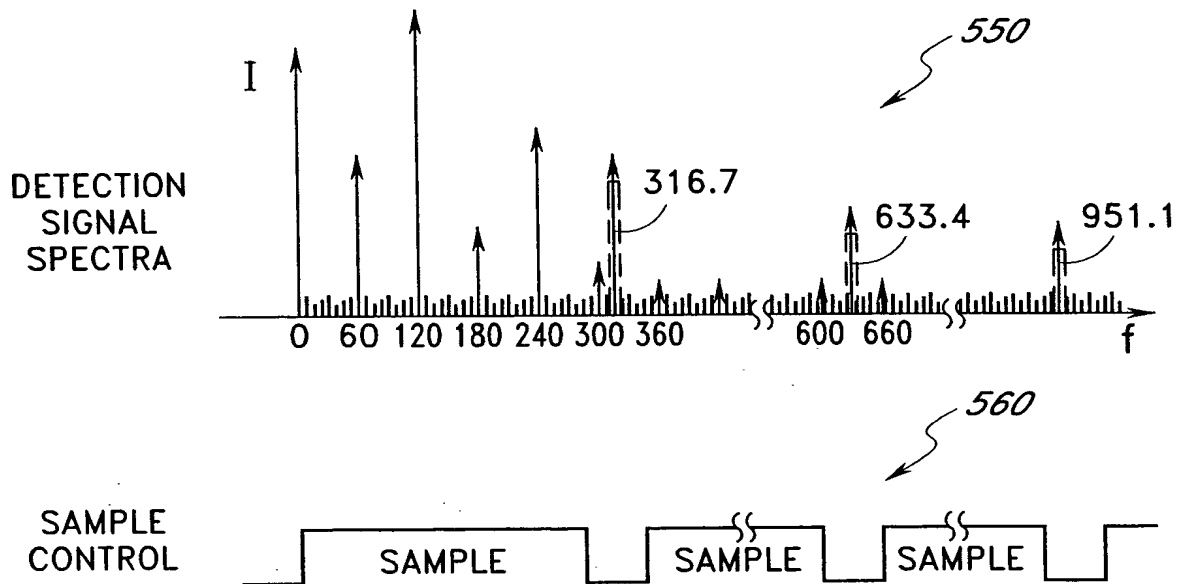


FIG. 14

METHOD AND APPARATUS FOR DEMODULATING SIGNALS IN A
PULSE OXIMETRY SYSTEM

Diab et al.

Appl. No.: Unknown

Atty Docket: MASIMO.CP1DV2

13/18

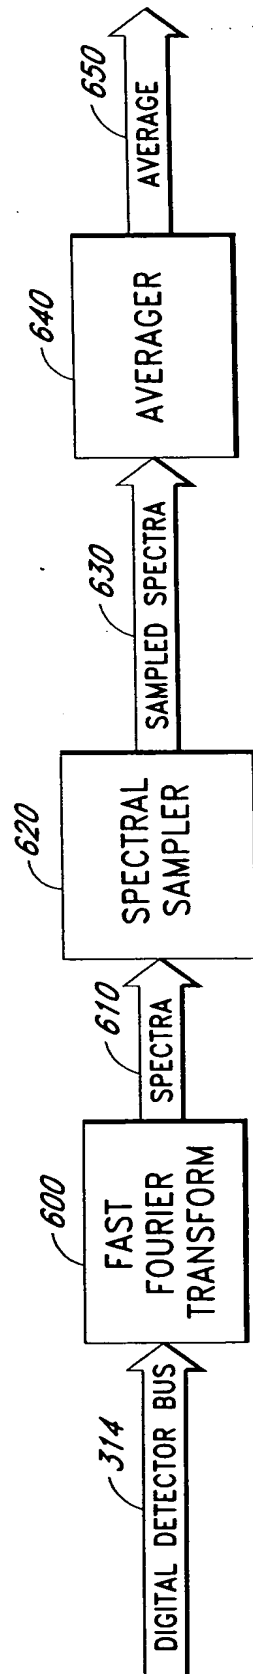


FIG. 15

METHOD AND APPARATUS FOR DEMODULATING SIGNALS IN A PULSE OXIMETRY SYSTEM

Diab et al.

Appl. No.: Unknown

Atty Docket: MASIMO.CP1DV2

14/18

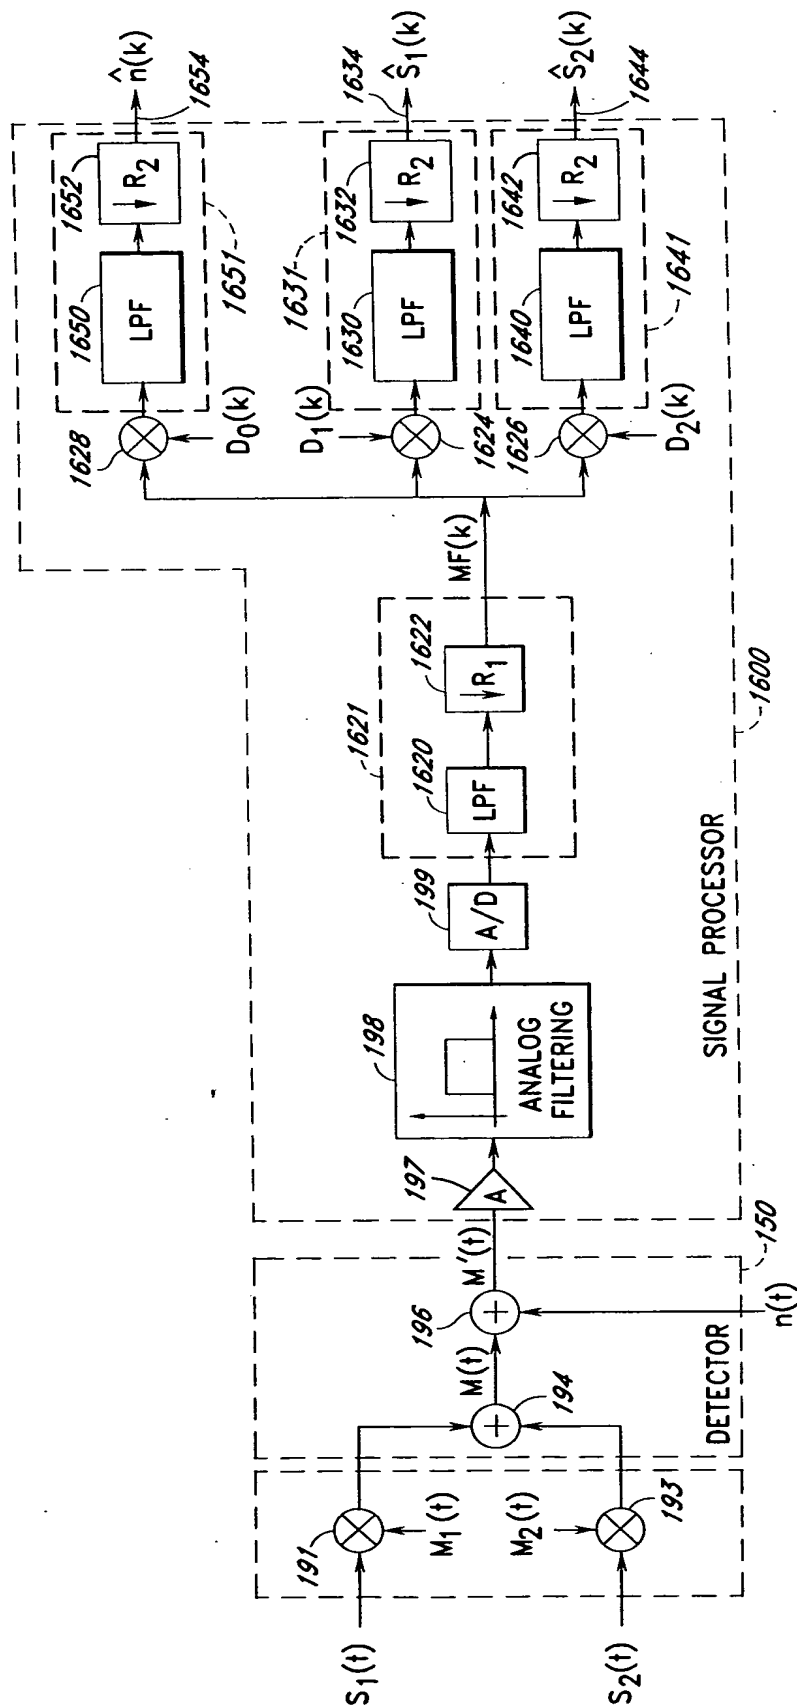


FIG. 16

METHOD AND APPARATUS FOR DEMODULATING SIGNALS IN A PULSE OXIMETRY SYSTEM

Diab et al.

Appl. No.: Unknown

Atty Docket: MASIMO.CP1DV2

15/18

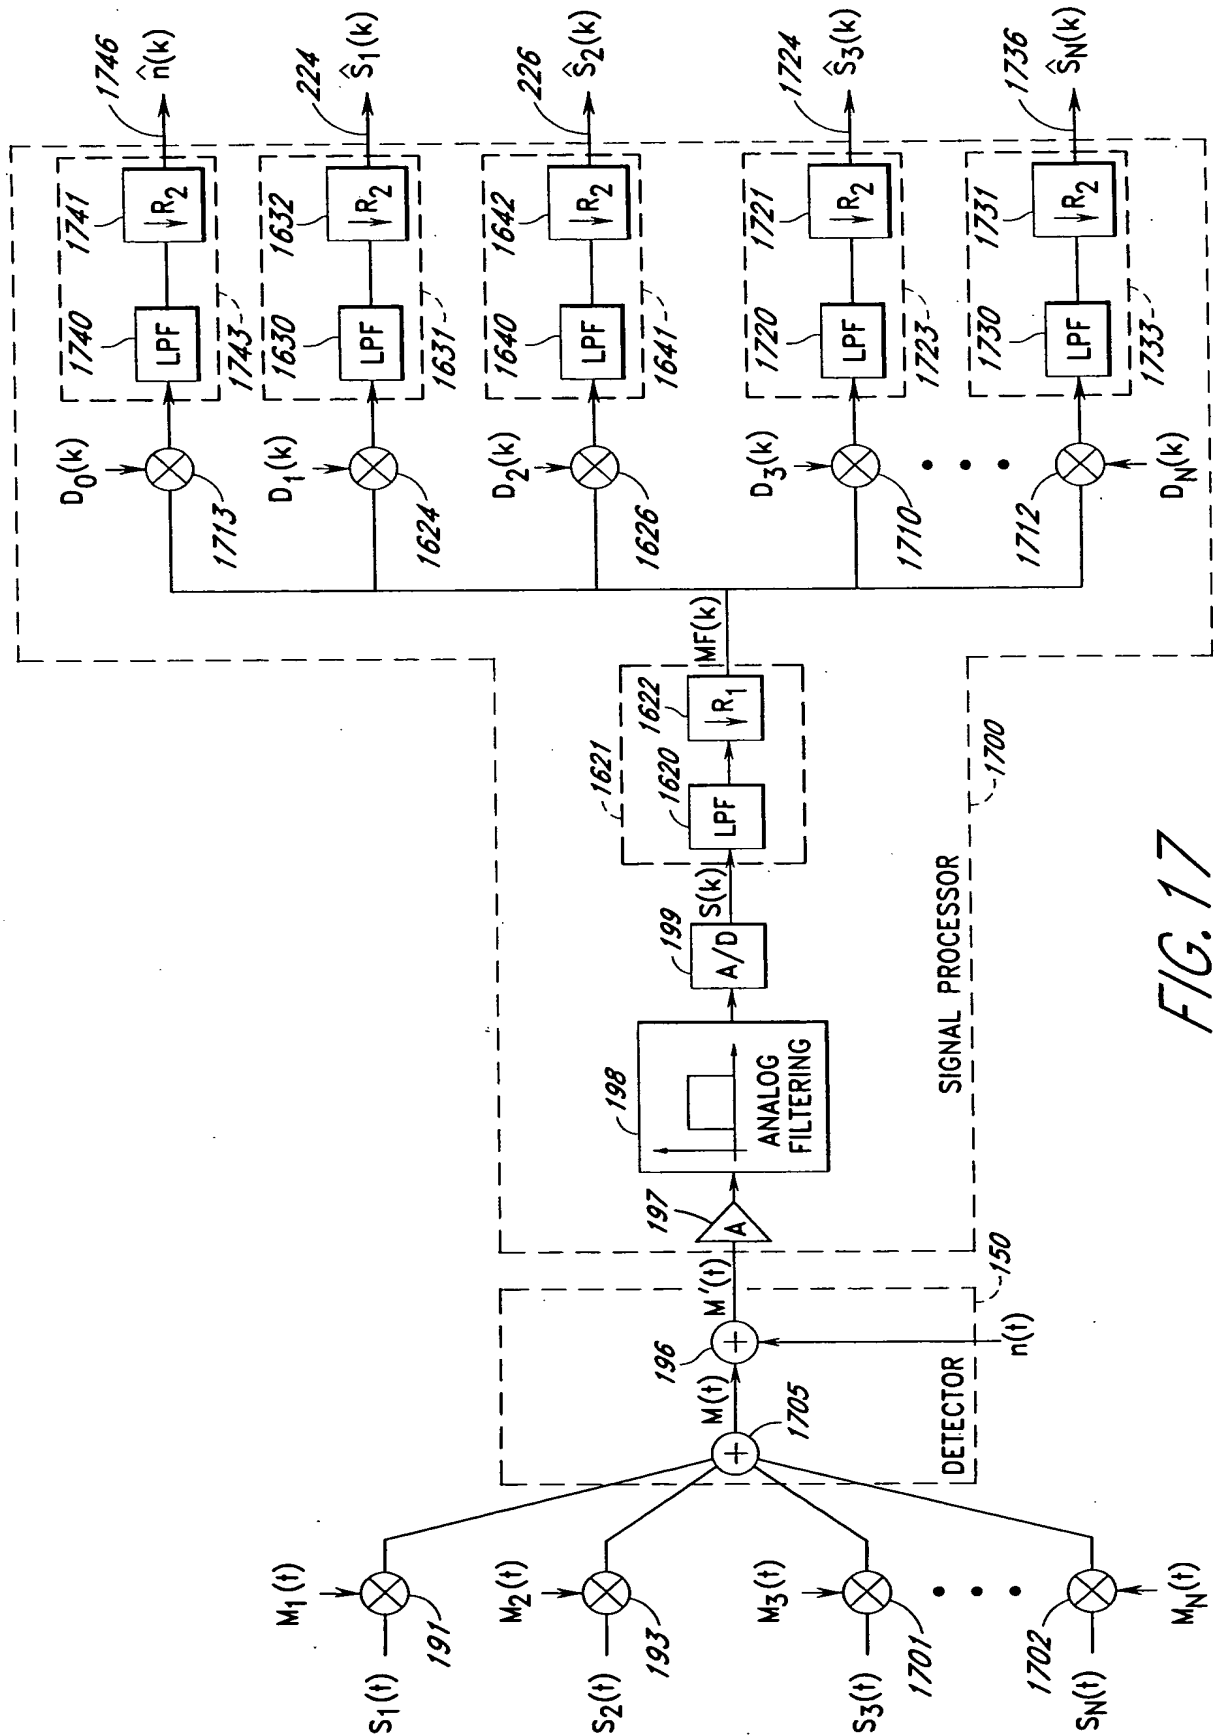


FIG. 17

METHOD AND APPARATUS FOR DEMODULATING SIGNALS IN A PULSE OXIMETRY SYSTEM

Diab et al.

Appl. No.: Unknown

Atty Docket: MASIMO.CP1DV2

16/18

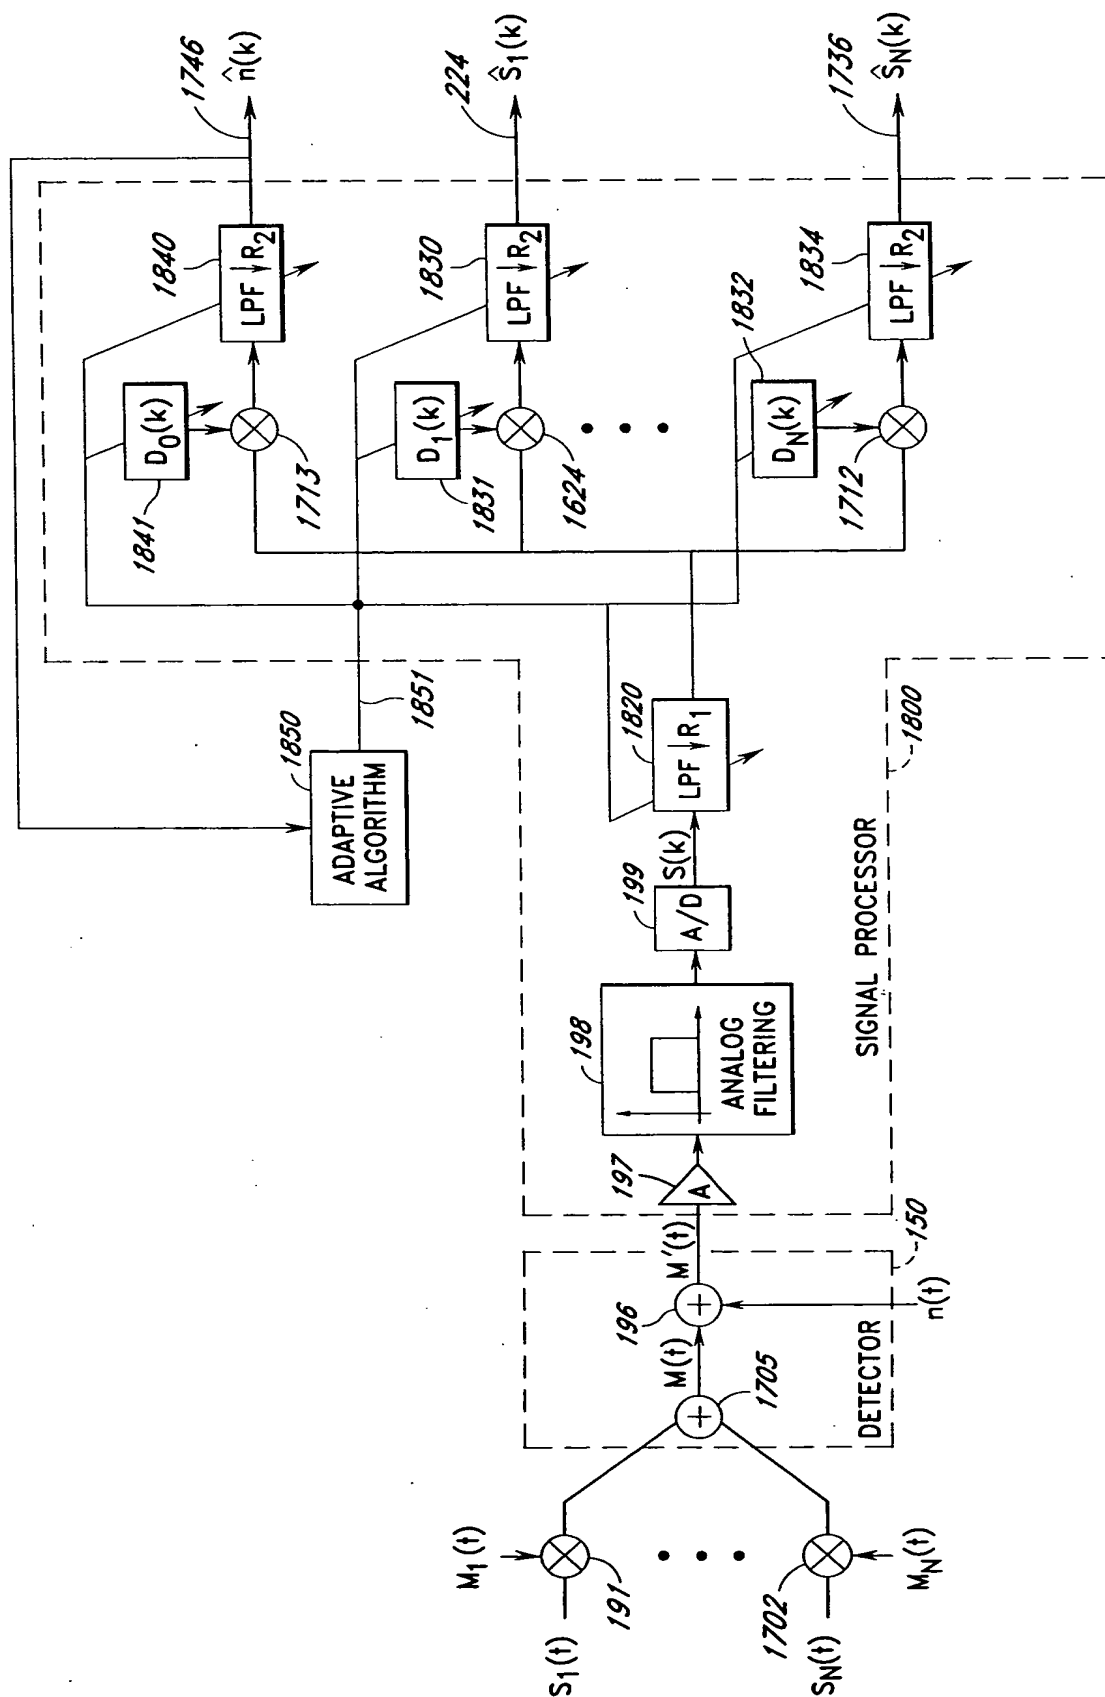


FIG. 18

17/18

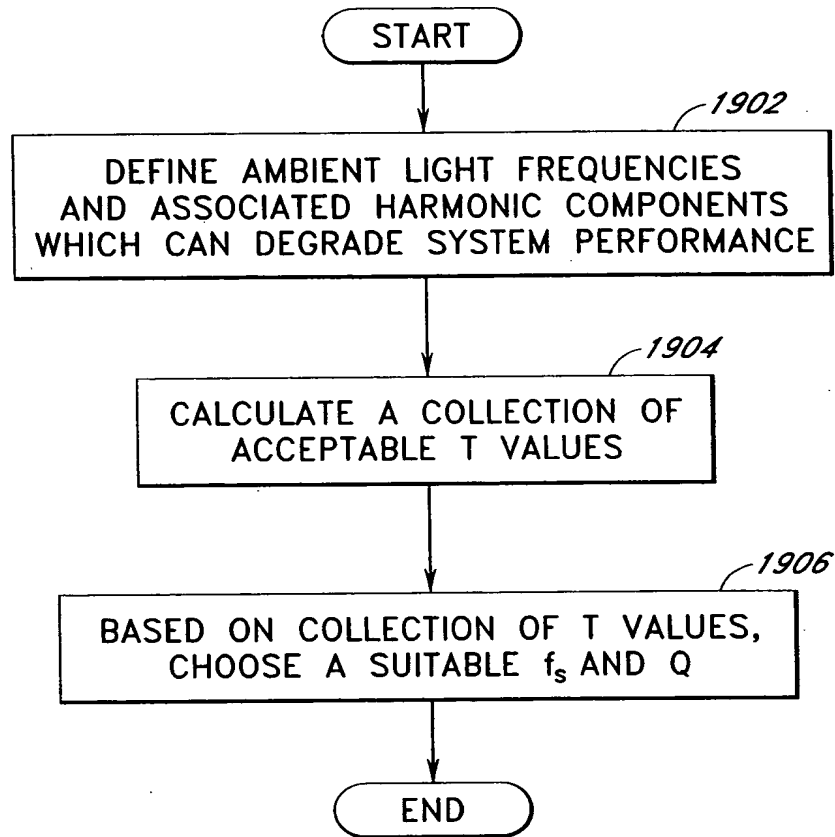


FIG. 19

METHOD AND APPARATUS FOR DEMODULATING SIGNALS IN A
PULSE OXIMETRY SYSTEM

Diab et al.

Appl. No.: Unknown

Atty Docket: MASIMO.CP1DV2

18/18

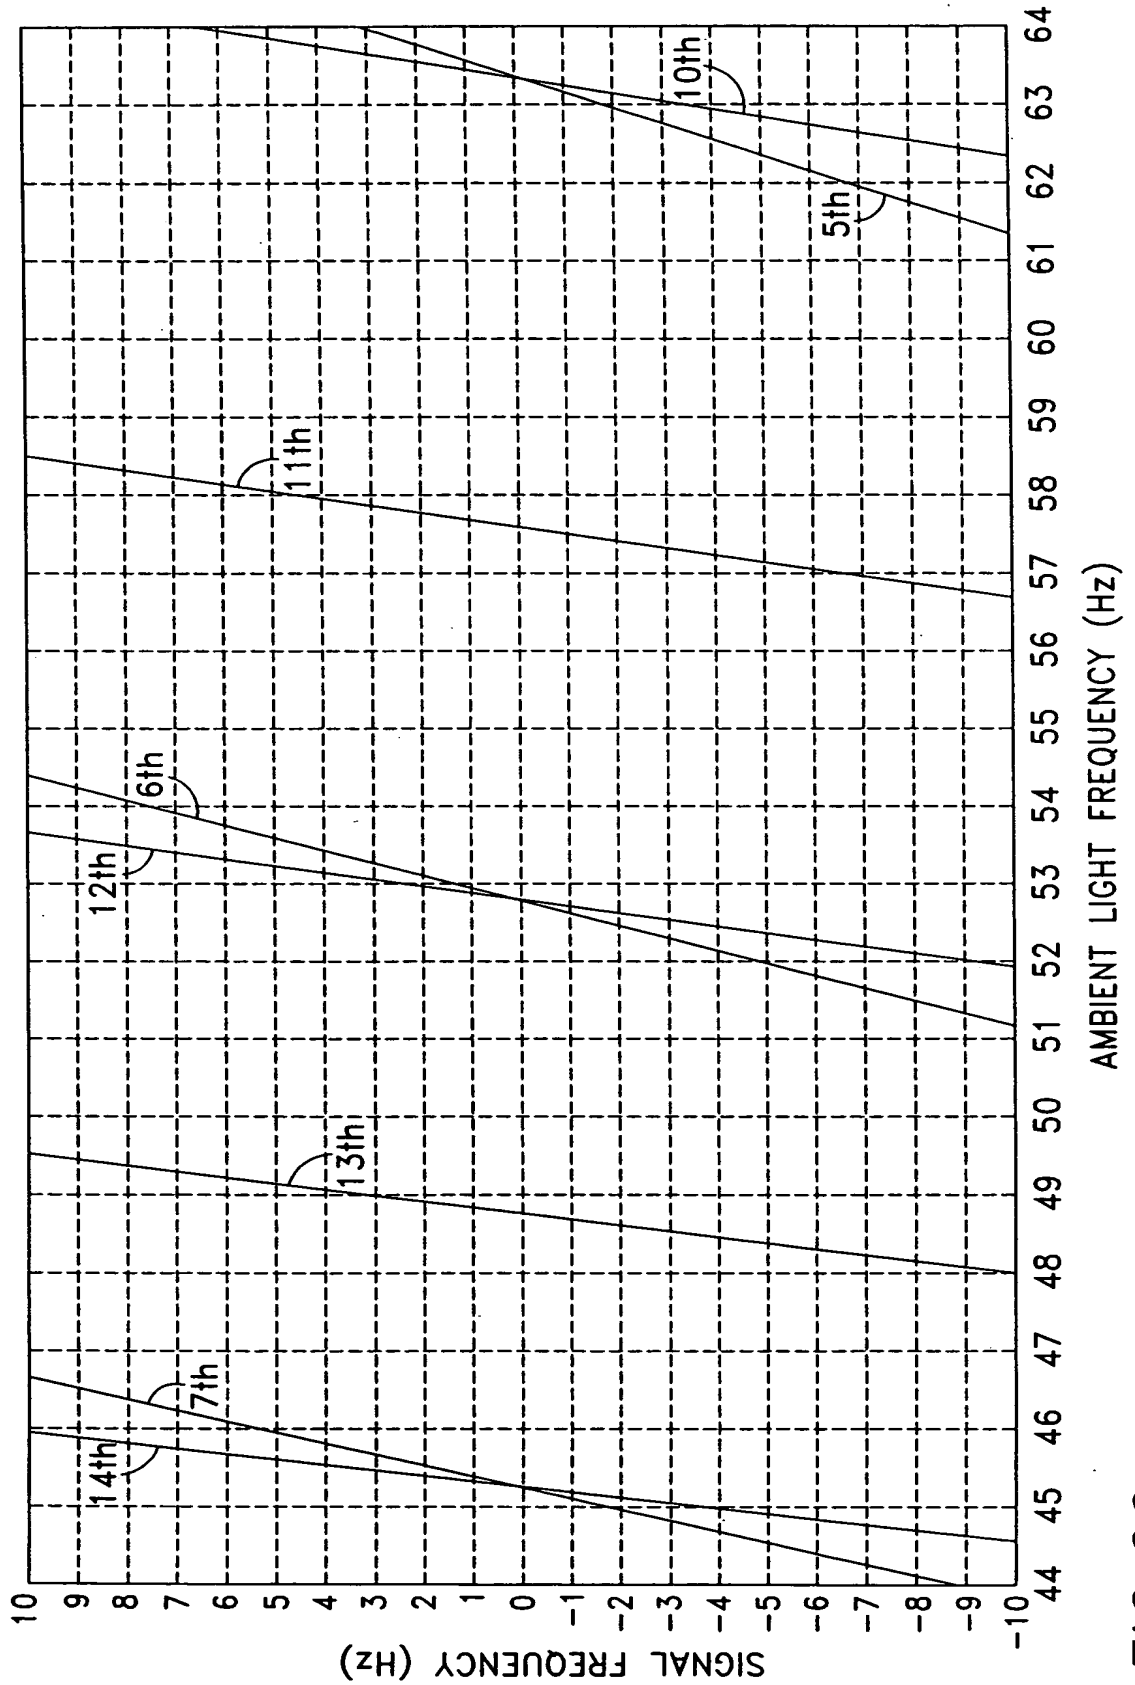


FIG. 20